

NEWS & VIEWS

Open Access

Water-insensitive down-shifting nanoparticles for sensitive biosensing

Jiang Ming¹, Sikun Hu¹ and Fan Zhang¹✉

Abstract

Conventional optical probes suffer from signal degradation in aqueous media, hindering sensitive biodetection. To overcome this, newly developed water-insensitive down-shifting nanoparticles (WINPs) possess superior photophysical properties in the NIR-I window, including high quantum yield and negligible thermal effects, permitting stable, high-contrast signal generation under low excitation power. This advantage facilitated a low-power lateral flow assay capable of highly sensitive avian influenza virus (AIV) detection in the opaque biological matrices (such as avian swabs), mitigating interference issues relying on visible-range signals.

Detecting biomarkers with high sensitivity and stability in complex biological fluids remains a significant challenge in diagnostics and biomedical imaging^{1,2}. Near-infrared (NIR) light offers advantages like deep tissue penetration and low autofluorescence, but the performance of lanthanide-doped upconversion nanoparticles (UCNPs), which convert NIR photons into higher-energy emissions through sequential absorption, is often hampered in aqueous environments^{3,4}. UCNPs typically rely on 980 nm laser excitation, which unfortunately coincides with strong water absorption, leading to detrimental signal quenching and localized heating effects that can damage sensitive biological targets and compromise assay reliability (Fig. 1a)⁵.

Overcoming these limitations requires novel nanoprobe designs that are inherently resilient to water-induced quenching and can operate efficiently at low, biologically safe power density levels. Down-shifting nanoparticles, which emit lower-energy photons upon absorbing higher-energy ones, present a promising alternative pathway for the NIR biological windows⁶. Recently, Kang et al. have developed and demonstrated Water-Insensitive Down-shifting Nanoparticles (WINPs) specifically for robust performance in water-rich

environments⁷. Core-shell nanoparticles (NaYF₄:5% Nd@NaYF₄) exhibit efficient absorption of 800 nm light and emit at 865 nm through an NIR-I-to-NIR-I down-shifting process (Fig. 1b).

Crucially, the researchers characterized the WINPs in the single-particle level. Their results confirmed their water-insensitivity: the photoluminescence lifetime profiles and the operational detection limit power density (a low 5 W cm⁻²) remained virtually identical whether the particles were measured in dry conditions or fully immersed in water. This starkly contrasts with conventional UCNPs, which showed lifetime reduction and required ~15 times higher power density to achieve a comparable signal in water due to energy transfer or absorption to water molecules. The WINPs achieved an impressive quantum yield of 22.1 ± 0.9%. Furthermore, excitation at 800 nm generated negligible thermal effects in water compared to the significant heating observed with 980 nm excitation under similar power densities (Fig. 1c).

Rapid and reliable detection of avian influenza virus (AIV) is critical for effective disease surveillance and outbreak control⁸. However, conventional lateral flow immunoassay (LFA) using colorimetric or fluorescent signals in the ultraviolet-to-visible spectrum often suffers from strong scattering and absorption in opaque and complex samples like avian swabs. Significant background interferences leading to compromised signal clarity and reduced detection reliability. To address

Correspondence: Fan Zhang (zhang_fan@fudan.edu.cn)


¹Department of Chemistry, State Key Laboratory of Molecular Engineering of Polymers, Laboratory of Advanced Materials, Shanghai Key Laboratory of Molecular Catalysis and Innovative Materials and iChem, Fudan University, Shanghai 200433, China

© The Author(s) 2025



Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.



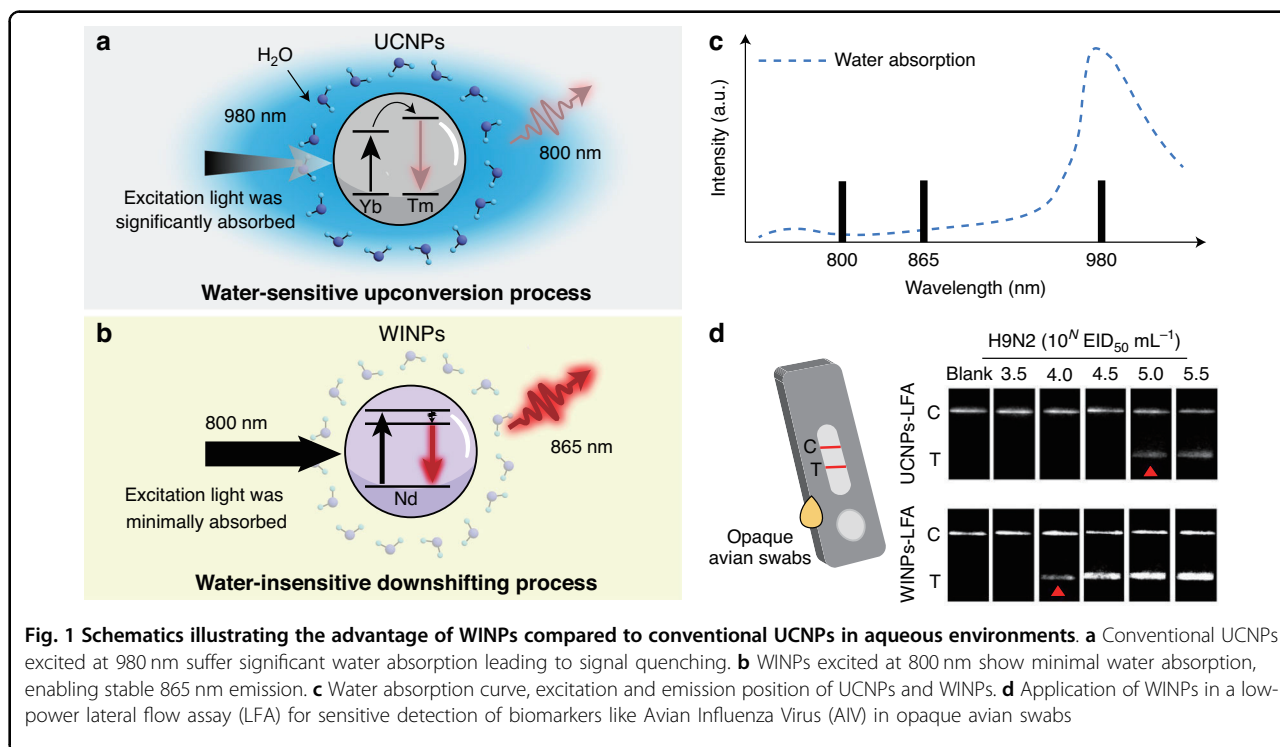

these limitations, they integrated the WINPs into an LFA platform for the specific detection of AIV nucleocapsid protein. Remarkably, the WINP-LFA demonstrated excellent performance even under a very low-power irradiation level (100 mW cm^{-2}). When tested against 65 opaque clinical samples, the assay achieved 100% sensitivity and specificity, with a detection limit about 10-fold lower than a comparable UCNP-based LFA tested under the same low-power conditions (Fig. 1d). Moreover, unlike conventional UCNPs systems that often require high excitation power leading to heat generation, WINPs provide stable, high-contrast signals without thermal drawback. This characteristic prevents heat-induced antibody denaturation and safeguards the overall reliability of the LFA.

This work addresses the challenge of water-induced luminescence quenching in NIR nanoprobes. By rationally designing an efficient NIR-I-to-NIR-I down-shifting system, the authors have created an interesting platform that functions at low power in aqueous environments. The WINP-LFA demonstrated their alternatives to conventional phosphors for developing cost-effective and sensitive biosensors. While the current NIR-I configuration demonstrates promising ex vivo sensing capabilities, its tissue penetration depth remains constrained by the fundamental optical properties of this

spectral region⁹. Developing next-generation nanoprobes with excitation/emission dual NIR-II (1000–1700 nm) operation, resistance to water absorption, and high brightness is crucial for enabling non-invasive in vivo biosensing^{10,11}.

Acknowledgements

This work was supported by the National Key R&D Program of China (grant no.2023YFB3507100), the National Natural Science Foundation of China (NSFC, grant nos.22104017, 22088101, and 22474026), New Cornerstone Science Foundation through the XPLOER PRIZE and the Research Program of Science and Technology Commission of Shanghai Municipality (Grant nos. 21142201000, 22JC1400400, and 20490710600), Innovation Program of Shanghai Municipal Education Commission (grant no. 2023ZKZD08) and China Postdoctoral Science Foundation (2025M771017, GZB20250253).

Conflict of interest

The authors declare no competing interests.

Published online: 05 September 2025

References

- Chen, Y., Wang, S. F. & Zhang, F. Near-infrared luminescence high-contrast in vivo biomedical imaging. *Nat. Rev. Bioeng.* **1**, 60–78 (2023).
- Barth, I. & Lee, H. Nanophotonic sensing and label-free imaging of extracellular vesicles. *Light Sci. Appl.* **14**, 177 (2025).
- Ming, J. et al. High-brightness transition metal-sensitized lanthanide near-infrared luminescent nanoparticles. *Nat. Photonics* **18**, 1254–1262 (2024).



4. Pei, P. et al. X-ray-activated persistent luminescence nanomaterials for NIR-II imaging. *Nat. Nanotechnol.* **16**, 1011–1018 (2021).
5. Wang, F. et al. Simultaneous phase and size control of upconversion nanocrystals through lanthanide doping. *Nature* **463**, 1061–1065 (2010).
6. Chang, Y. L. et al. Bright Tm^{3+} -based downshifting luminescence nanoprobe operating around 1800 nm for NIR-IIb and c bioimaging. *Nat. Commun.* **14**, 1079 (2023).
7. Kang, D. et al. Water-insensitive NIR-I-to-NIR-I down-shifting nanoparticles enable stable biomarker detection at low power thresholds in opaque aqueous environments. *Light Sci. Appl.* **14**, 235 (2025).
8. Jeon, E. et al. Biporous silica nanostructure-induced nanovortex in microfluidics for nucleic acid enrichment, isolation, and PCR-free detection. *Nat. Commun.* **15**, 1366 (2024).
9. Wang, T. et al. A hybrid erbium(III)-bacteriochlorin near-infrared probe for multiplexed biomedical imaging. *Nat. Mater.* **20**, 1571–1578 (2021).
10. Yang, Y. W. et al. Fluorescence-amplified nanocrystals in the second near-infrared window for in vivo real-time dynamic multiplexed imaging. *Nat. Nanotechnol.* **18**, 1195–1204 (2023).
11. Fan, Y. et al. Lifetime-engineered NIR-II nanoparticles unlock multiplexed in vivo imaging. *Nat. Nanotechnol.* **13**, 941–946 (2018).

